Introduction

Your Veeder-Root brand C628 Totalizer is one model in a family of 1/8 DIN units which offers breakthrough display technology as well as easy-to-program single-line parameters. Designed to provide instant visual feedback regarding an application's key input value, the C628 not only has a 0.71" high LED display (27% larger than other 1/8 DIN units), but also the ability to change display color based on process status (programmable parameter in Operation Mode). Easy programming is made possible via a help function and a secondary legend display.

This manual will guide you through the installation and wiring of your C628 unit with information on proper panel mounting and rear terminal layout and wiring instructions. In addition, the instrument's operation and programming modes are thoroughly explained. The Operation Mode provides day to day operation and allows editing of preset values. The Program Mode enables the configuration of various parameters prior to initial operation. These parameters include those for basic configuration as well as other settable features which will enhance the functionality and usability of the device.

This manual also provides information on the C628 Totalizer's product specifications and ordering and warranty procedures.



Features

- AWESOME 0.71" high digit LED display
- Programmable color change display based on an event
- Programmable help function and secondary legend display
- Choice of NPN or PNP primary input
- Filter speed settable for 20, 200, or 10,000 Hz
- · Front panel reset enable and preset lockout
- Optional RS-485 plug in card
- CE approved


Index

Installation	
Panel Mounting	page 2
Wiring	page 3
Operation	
Front Panel	page 4
Operation Mode	page 5
Programming	
Program Mode	page 6-9
Appendix A	
Specifications	page 10
General	
Notes	page 11
Ordering Information	page 12
Warranty	page 12

Technical Manual 702138-0001

Veeder-Root brand Series C628 Totalizer (C628-1XXX)

INSTALLATION

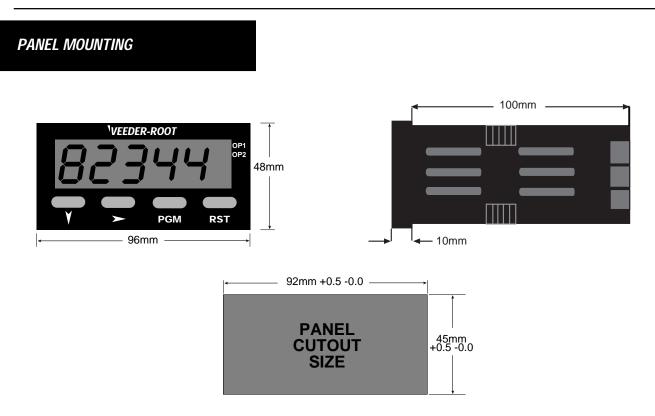

Mounting Grooves drawing above drawing drawi

The instrument can be mounted in a panel with a thickness of up to 6mm. The cutout(s) should be made based on the recommended panel opening illustrated in the drawing above.

Insert the unit in the panel through the cutout. Ensure that the panel gasket is not distorted and the instrument is positioned squarely against the panel. Slide the mounting clamp into place on the instrument, as shown to the left, and push it forward until it is firmly in contact with the rear face of the mounting panel and the tabs on the bracket arm are seated in the mounting grooves on the side of the unit.


The electronic components of the instrument can be removed from the housing after installation without disconnecting the wiring. To remove the components, grip the side edges of the panel and pull the instrument forward. Take note of orientation of the unit for subsequent replacement in the housing.

Bracket Arm

INSTALLATION

WIRING

REAR TERMINAL CONNECTIONS

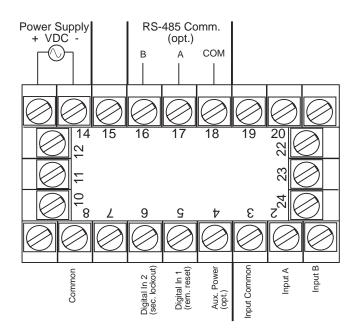

Count Inputs

Terminal #2 is the connection for Input A, which is programmable to be the primary input or channel A of an encoder input. Terminal #1 is the connection for Input B, which is programmable to be an incrementing input, a decrementing input, or channel B of an encoder input. The common connection for both Input A and Input B is Terminal #3.

Control/Digital Inputs

A contact closure or NPN signal can be used to activate preconfigured functionality. Terminal # 5 is used for a remote reset function, while Terminal #6 is a security function, that when active, will prohibit entry into Program Mode. Terminal #8 serves as the common for both of these inputs.

Auxiliary Power Output

A 9 - 15 VDC for powering external sensors and encoders up to 125 mA can be accessed by connecting the positive supply side of the sensor to Terminal #4 and the negative side to Terminal #8.

Input Power


For an AC powered unit, Terminal #13 serves as the line or Hot side connection for AC powered units and as the positive side for DC powered units. The neutral side for AC powered units and the negative side for DC powered units are connected to Terminal #14.

Serial Communication

An RS-485 communication board, utilizing ASCII protocol, can be installed as an option. Terminals #16 & #17 serve as the B and A connections respectively, while Terminal #18 is connected as the common.

Terminals 7, 9, 10, 11, 12, 15, 19, 20, 21, 22, 23, & 24 are not used.

OPERATION

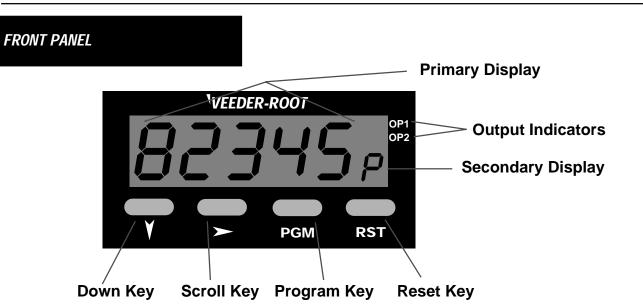

Key Functions

Key	Function
Down	<i>In Operation Mode</i> : Used in edit operation to decrement the digit highlighted by the Scroll key.
	<i>In Program Mode</i> : Used in Edit Operation to decrement the digit highlighted by the Scroll key, if the setting is a numerical value, or present the next in the series of choices for that parameter.
Scroll	<i>In All modes</i> : Moves the unit into Edit Operation, which is indicated by the left most digit flashing. Successive presses of the key are used to move to the digit to be edited. Wrap around will occur from least significant digit to most significant digit.
Program	<i>In Operation Mode</i> : Used to move between the count value display & the preset and to enter an edited preset value. Holding the key down for 3 seconds will cause the unit to enter Program Mode.
	<i>In Program Mode</i> : Used to move from one parameter to the next and enter the edited parameter values. Holding the key down for 3 seconds will cause the unit to return to Operation Mode.
Reset	<i>In Operation Mode</i> : Resets the count value to zero (or to the preset in count down operation). This button can be disabled via the "Front Panel Reset Enable" parameter in Program Mode.
	In Program Mode: No function.
Down & Scroll together	<i>In All modes</i> : Will abort an Edit Operation and return the preset/parameter to its previous value.
4	1

Display Functions

Display Functions		
Display	Function	
Primary	<i>In Operation Mode</i> : Default display is the count value. Can be scrolled using the program key to display the Preset value. If the "Help" function is enabled, this display will first show the parameter description for 3 seconds (see page 5 for example).	
	<i>In Program Mode:</i> Displays the value or selection for the current parameter. If the "Help" function is enabled, this display will first show the parameter description for 3 seconds (see page 6 for example).	
Secondary	<i>In Operation Mode</i> : Indicates alphabetically if the Preset is being viewed on the primary display. This display is blank when the Count Value is being shown.	
	<i>In Program Mode:</i> Provides a 1 digit alpha or numeric character to indicate which parameter value is being shown on the primary display.	
Output Indicators	In All modes: No function.	

OPERATION

OPERATION MODE

CHANGING A PRESET VALUE



PGM

PGM

Default display is the present count value.

Pressing the Program Key will cause the

main display.* If there is no key activity

for 3 seconds, the primary display will

Continued pressing of the Program Key

switch back to the count value.

display description to appear on the





PGM PGM



Use the Scroll Key to move from left to right and highlight the digit that needs to be changed. Wrap around will occur from the least significant to the most significant digit.

Use the Down Key to decrement the digit until the desired value appears. The display will wrap around from 0 to 9.

After the desired digits have been changed, press the Program Key to enter the new value. The new value will appear on the main display without any flashing digits. Press the Progam Key again and the parameter description will appear on the main display.

* Parameter descriptions will not appear on the primary display if the "Help" function has been disabled. ** Edit Operation cannot be accessed if the Preset Lock has been enabled in Program Mode.

VEEDER-ROOT

will scroll to the Preset. (See Parameter Sequence below.) The full parameter description will appear on the main display.* To change the Preset value, press the

Scroll Key. If there was no key activity for 3 seconds, the Preset value will appear (one digit description shown on secondary display); however, press the Scroll Key in order to edit. The unit will now be in Edit Operation as signified by the most significant digit flashing.**

PARAMETER SEQUENCE



PGM

Count

Function: Displays present count value *Range:* 0 to 99999



Preset

Function: Sets preset value - only used to change the display color

Adjustment Range: 0 to 99999

Default Value: 10

PROGRAM MODE

ENTERING PROGRAM MODE AND BASIC OPERATION

The Program Mode can be accessed from the Operation Mode by holding the Program Key for 3 seconds.

The name of the first parameter will appear	
on the primary display.*	

Successive presses of the Program Key will scroll the display through the remaining parameters in the Program Mode. To exit Program Mode, hold the Program Key for 3 seconds.

* Parameter names will not appear on the main display if the "Help" function has been disabled in Program Mode.

Y → PGM RST PGM for 3 seconds VEEDER-ROOT VEEDER-ROOT PGM RST



PGM




Edit Operation



Pressing the Scroll Key or no key activity for 3 seconds will display the value for that parameter. The secondary display will indicate the one digit identifier for the parameter. The digit in the secondary display will flash to indicate the unit is in Program Mode. If the Scroll Key was pressed (instead of waiting 3 seconds), the unit is in Edit Operation, as indicated by the MSD flashing. If there had been no key activity for 3 seconds, press the scroll key to enter Edit Operation (MSD flashing). Use the scroll and edit buttons to change the value as in Operation Mode, described on page 5. Press the Program Key to enter any changes.

PARAMETER SEQUENCE



Calibration Factor

Function: Used to scale the input into engineering units by multiplying this value by the number of pulses received

Adjustment Range: 0.0001 to 9.9999 Default Value: 1.0000

Decimal Position


Function: Set the decimal point position for the count and preset displays *Adjustment Range:* 0 to 0.0000 *Default Value:* 0

PROGRAM MODE Continued



Count Mode

Function: Defines how the input pulses will be applied to the count value Adjustment Range:



A & B channels

increment the total

Default Value: A+B



A-B: Inputs on the A Directional: When input channel increment the B is inactive, input A total, while inputs on the increments. When input B channel decrement B is active, input A decrements



Quadrature: The unit accepts a phased input from an encoder. The total increments when the A channel leads the B channel

6 R ن 9



PGM

SPEEdr

Input Type

Function: Programs the unit to match the electrical characteristics of the input signal



Sinking: The unit will accept a NPN or dry contact input which sinks voltage to common

Source: The unit will accept an PNP input which sources voltage

Src

Default Value: Sinking

Filter Speed

Function: Enables the debounce filter of the counter to properly match the application

Adjustment Range:



20: The unit will accept up to 20 pulses per second. Generally used with contact inputs to eliminate false counts caused by contact bounce 200

up to 200 pulses per

second. Generally used

for higher speed contact

inputs or to filter noise

on electronic signals in

low speed applications

10000

200: The unit will accept 10,000: The unit will accept up to 10,000 pulses per second. Generally used with high speed electronic inputs and encoders



Default Value: 10000

PROGRAM MODE Continued



Front Panel Reset Enable

Function: Determines whether the Front Panel Reset key can be used to reset the count value Adjustment Range:





Enable: The count value can be reset while being viewed in Operation Mode by pressing the Front Panel Reset Key

Default Value: Enable

Disabled: The Front Panel Reset Key is disabled and the count value can only be reset through the Remote **Reset Input**





Serial Communication Enabled

Function: Activates the RS-485 communication option board

Adjustment Range:



None: No communication Fitted: A communication board installed board is installed in the unit

Default Value: If ordered from the factory with the RS-485 board, the default will be "fitted". If the board is installed in the field, this parameter will need to be changed from its default of "none"

Communication Address (Appears only if communication board is installed and activated)





PGM



PGM

Baud Rate (Appears only if communication board is installed and activated)

Function: Defines the unique communication address of the counter

Function: Selects the serial communication speed

Adjustment Range:

Default Value: 1



Adjustment Range: 1 to 99



2400 BPS

4800 BPS



9600

9600 BPS

Default Value: 4800



8





Display Color Change

Function: Defines the color of the display for prior to and after the preset value is reached Adjustment Range:

	rEd
Red:	The display will

always be red



- GrEEn Green: The display will always be green
- Green to Red: The display will be green prior to the Preset value being reached. It will turn red after the Preset has been reached

Ũn_rd



Red to Green: The display will be red prior to the Preset value being reached. It will turn green after the Preset has been reached



 $\boldsymbol{\varphi}$

Locy

Preset Lock

Function: Determines whether the Preset Value can be changed via the front panel



Default Value: Green to Red

18 -Enable: Preset value is 5 ، ک

read only Default Value: Disable Disabled: Preset value can be viewed and changed






Help Prompt

Function: Determines whether the multi-character parameter name will appear on the main display for 3 seconds prior to the parameter value appearing

Adjustment Range:

HLP 9



Help - No: Only the parameter values will appear on the primary display. The parameter can be identified by a single digit in the secondary display

Default Value: Help - Yes



APPENDIX A

SPECIFICATIONS

Count Inputs

 $\begin{array}{lll} Type: & Sinking/Sourcing \mbox{ or Contact Closure} \\ Frequency: & 10 \mbox{ kHz max}. \\ Logic: & Low \leq 2.0 \mbox{ VDC}, \mbox{ High} \geq 3.0, \mbox{ 30V max}. \\ Impedance: & 10 \mbox{ K}\Omega \mbox{ to common - Sourcing} \\ 4.7 \mbox{ K}\Omega \mbox{ to +Voltage - Sinking} \\ \end{array}$

Control Inputs

Type: Logic: Impedance: Response Time: Function: Sinking, Edge Sensitive Low ≤ 2.0 VDC, High ≥ 3.0 4.7 K Ω to +Voltage 25 ms Input 1: Remote Reset Input 2: Security Lockout

Approvals

General:	CE	
EMC Susceptibility:	Complies with EN50082-1:	1992,
1 5	EN50082-2: 1995	
EMC Emissions:	Complies with EN50081-1:	1992,
	EN50081-2: 1994	
Safety:	Complies with EN61010-1:	1993

Communication

Type:Serial asynchronous, UART to UARTData Format:Open ASCII: One start bit, even parity seven
data bits, one stop bitPhysical Layer:RS-485Maximum Zones:99Baud Rate:Selectable from 9600, 4800, 2400, or 1200

Electrical

Supply Voltage: 90-264 VAC, 50/60 Hz, or 20-50 VAC/VDC Power Consumption: 4 Watts Access. Power Supply:9-15 (unregulated VDC), 125 mA max.

Display

```
Type:
Height:
```

Red/Green, 7 segment LED, 5 digits primary display, single digit secondary display 0.71" (18mm) primary display, 0.3" (7mm) secondary display

Physical

Dimensions: Mounting:

Terminals: Front Panel Rating: Case Material: Weight: 48mm x 96mm, 110mm deep Panel mount (mounting bracket supplied), 45mm x 92mm cutout Screw type - combination head NEMA 4X/IEC IP65 GE Lexan 940 0.56 lbs.

Environmental


Operating Temp.: Storage Temp.: Relative Humidity: 0° to 55° Celsius, 32° to 131° Fahrenheit -20° to 80° Celsius, -4° to 176° Fahrenheit 20% to 95% non-condensing

GENERAL

NOTES		

GENERAL

ORDERING INFORMATION

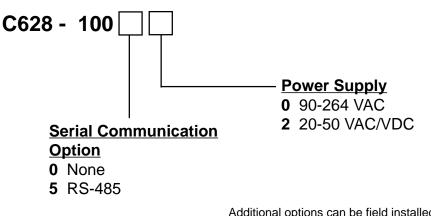

Additional options can be field installed through plug-in boards which can be ordered separately.

Description	Part #
RS-485 Comm. Board	T50-005

WARRANTY

Standard products manufactured by the Company are warranted to be free from defects in workmanship and material for a period of one year from the date of shipment, and products which are defective in workmanship or material will be repaired or replaced, at the option of the Company, at no charge to the Buyer. Final determination as to whether a product is actually defective rests with the Company. The obligation of the Company hereunder shall be limited solely to repair and replacement of products that fall within the foregoing limitations, and shall be conditioned upon receipt by the Company of written notice of any alleged defects or deficiency promptly after discovery within the warranty period, and in the case of components or units purchased by the Company, the obligation of the Company shall not exceed the settlement that the Company is able to obtain from the supplier thereof. No products shall be returned to the Company without its prior consent. Products which the Company consents to have returned shall be shipped F.O.B. the Company's factory. The Company cannot assume responsibility or accept invoices for unauthorized repairs to its components, even though defective. The life of the products of the Company depends, to a large extent, upon the type of usage thereof, and THE COMPANY MAKES NO WARRANTY AS TO FITNESS OF ITS PRODUCTS FOR SPECIFIC APPLICATIONS BY THE BUYER NOR AS TO PERIOD OF SERVICE UNLESS THE COMPANY SPECIFICALLY AGREES OTHERWISE IN WRITING AFTER THE PROPOSED USAGE HAS BEEN MADE KNOWN TO IT.

THE FOREGOING WARRANTY IS EXCLUSIVE AND IN LIEU OF ALL OTHER WARRANTIES EXPRESSED OR IMPLIED, INCLUDING, BUT NOT LIMITED TO ANY WARRANTY OF MERCHANTABILITY OR OF FITNESS FOR A PARTICULAR PURPOSE.



Printed in U.S.A. 702138-0001 March 1998 Revision none